


[Preparing to do the test]

1. Keep a clock, timer or stopwatch at hand.
2. **Ensure that all test components are kept at room temperature (15-30 °C).**
3. Ensure that the packaging is intact; Do not use the test if there is visible damage of the foil packaging.
4. Open the box and you will get the components shown below:

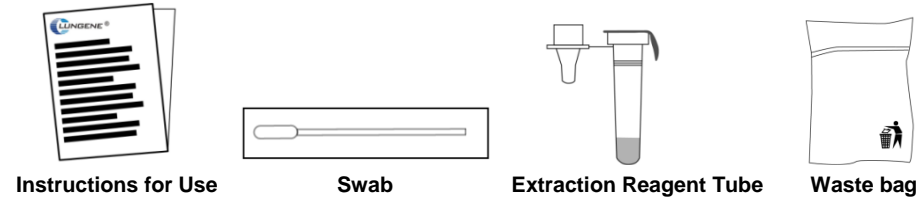


Test Cassette

Note: Only open the foil packaging of the test cassette when you are ready to carry out the test. Use the test cassette within one hour after opening.

[Before starting]


Wash your hands in soapy water and dry thoroughly.



[Step-By-Step Instructions]


1. Open Extraction Reagent Tube

Carefully tear off the sealed foil film on the extraction reagent tube.

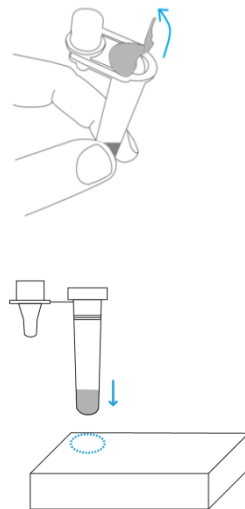


2. Insert Tube into Box

Gently press the tube through the perforated hole in the box.




3. Remove the Swab

- a. Open the swab package at the stick end.




Note: Keep fingers away from swab tip.

- b. Take out the swab.





4. Swab the Left Nostril

- a. Gently insert the entire tip of the swab, app. 2.5 cm into the left nostril.




- b. Firmly brush the swab against the inside of the nostril in a circular motion 5 times or more.




(Approximately 1.5 times the length of the swab tip)

5. Swab the Right Nostril

- a. Remove the swab from the left nostril and insert it into right nostril about 2.5 cm.



- b. Firmly brush the swab against the inside of the nostril in a circular motion 5 times or more.




CHECK!
You should swab both nostrils.

Note: A false negative result may occur if sample collection is not thoroughly undertaken.


6. Insert the Swab into the Tube

Insert the nasal swab into the tube which contains the extraction reagent.




7. Rotate the Swab 5 Times

- a. Rotate the swab at least 5 times while pressing the swab tip against the bottom and the sides of the tube.




- b. Let the tip of the swab soak in the tube for 1 minute.




8. Remove the Swab

- a. Remove the swab while squeezing the sides of the tube against the swab, to release the liquid from the swab.

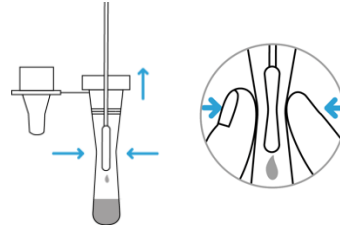


- b. Cover the tube with the provided cap tightly and insert the tube back into the box.




9. Take out the Test Cassette from the pouch

Open the sealed pouch and take out the test cassette.



Note: Test cassette must lay **FLAT** on the table during the entire testing.



10. Add Sample to the Sample Well

- a. Hold the tube vertically over the Sample Well - not at an angle.



- b. Add 3 drops from the tube into the Sample Well by gently squeezing the sides of the tube.

Note 1: A false negative result may occur if less than 3 drops of sample is used.


Note 2: The result will not be affected if 1-2 more drops of sample are accidentally added – as long as you can read a C-line (see Read result below).

11. Timing

Start the clock / stopwatch or timer.

12. Wait 15 Minutes

Read the test result at 15-20 minutes, **DO NOT** read the result after 20 minutes.

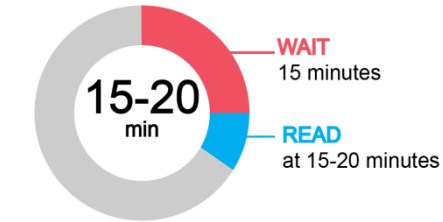

Note: False results can occur if the test results are read before 15 minutes or after 20 minutes.

[Read result]

Positive Result

Two lines appear. One coloured line appears at the control region (C), and another appears at the test region (T).



Please look very closely!

The intensity of the T-line can be very faint.

A positive test result indicates that you are likely to carry the COVID-19 disease. Contact your State or Territory Coronavirus testing services to **get a laboratory PCR test** as soon as possible, and follow local guidelines for self-isolation to avoid spreading the virus to others.

Negative Result

One coloured line appears at the control region (C), and no line appears at the test region (T).



A negative test result indicates that you are unlikely to carry the COVID-19 disease. Even if you get a negative result, you still need to follow all public health advice on limiting the spread of COVID-19.

Please contact your State or Territory Coronavirus testing services to get a laboratory PCR test if you develop symptoms or symptoms are persisting. If you suspect an infection, it is recommended that you repeat testing after 1-2 days, as the virus cannot be precisely detected in all phases of an infection.

Invalid Result


Control (C) line fails to appear.



Note: If a C-line does not appear, the test result is invalid regardless of the appearance of a T-line or not.

If a C-line does not appear, you need to retest with a new test cassette or contact your State or Territory Coronavirus testing services to get a laboratory PCR test.

[Dispose of the used test kit]



Collect all parts of the test kit and place in the waste bag that can be placed in the general waste.

Wash your hands thoroughly after handling.